


NANOCOLOR® Härte Ca/Mg

Hardness Ca/Mg / Dureté Ca/Mg / Durezza Ca/Mg













Test 0-44
REF 985044

Methode / Method / Méthode / Método

0443 1.0–20.0 °d
5–50 mg/L Mg²⁺
10–100 mg/L Ca²⁺


540/570 nm

Min	20–80 %		Max
5	14	41	50 mg/L Mg ²⁺
10	28	82	100 mg/L Ca ²⁺

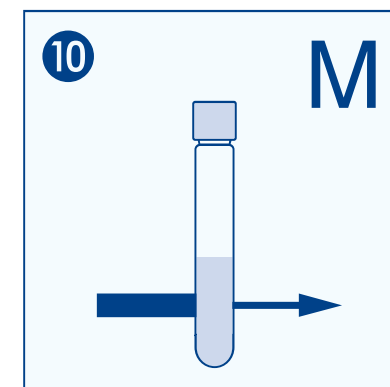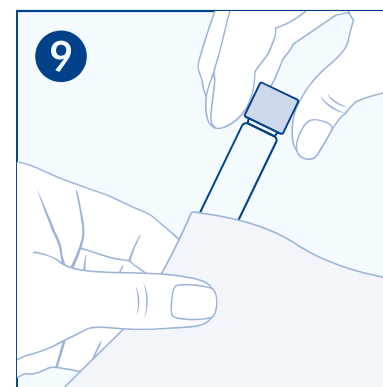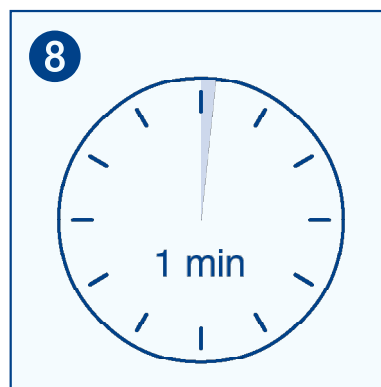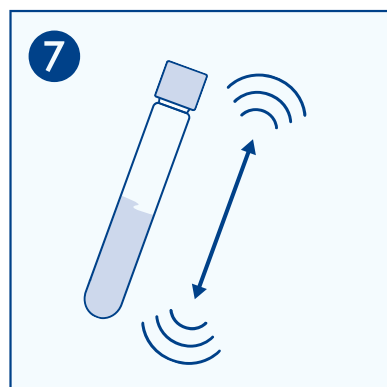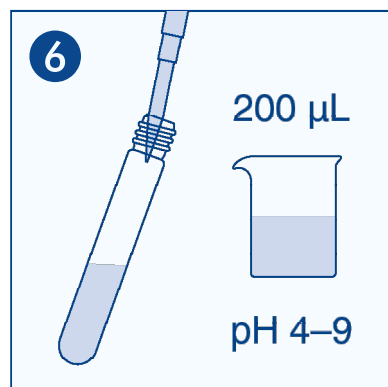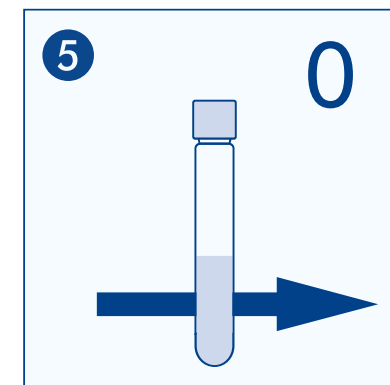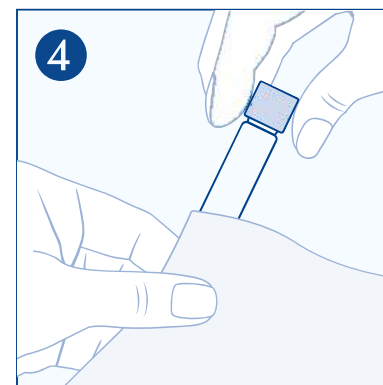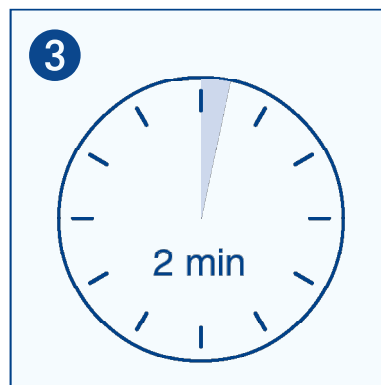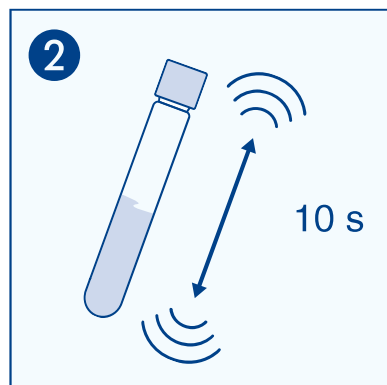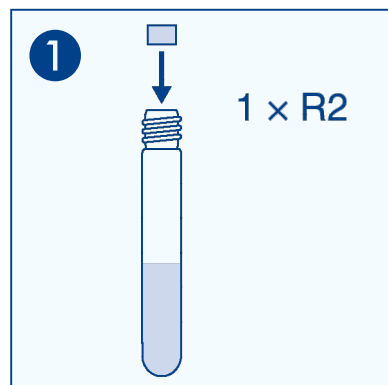

NANOCOLOR® Härte Ca / Mg

Hardness Ca / Mg / Dureté Ca / Mg / Durezza Ca / Mg



Test 0-44
REF 985044

Methode / Method / Méthode / Método

540 / 570 nm

0444 1.0 – 25.0 °e
 0445 2.0 – 36.0 °f
 0446 0.2 – 3.6 mmol/L
 0447 20 – 350 mg/L CaCO₃

Min	20 – 80 %	Max
5	14 41	50 mg/L Mg ²⁺
10	28 82	100 mg/L Ca ²⁺

