


MACHEREY-NAGEL

# User manual

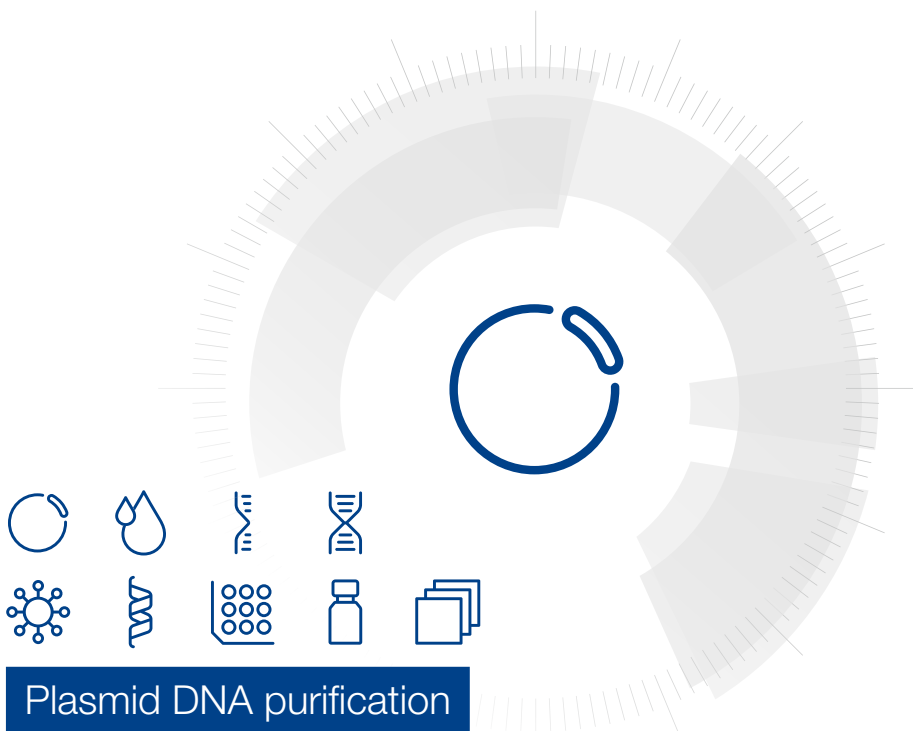



## Plasmid DNA purification

- NucleoBond® Xtra Midi
- NucleoBond® Xtra Maxi
- NucleoBond® Xtra Midi Plus
- NucleoBond® Xtra Maxi Plus

October 2024 / Rev. 19

# Plasmid DNA purification (NucleoBond® Xtra Midi / Maxi)

## Protocol at a glance (Rev. 19)

|   | Midi  |   | Maxi  |   |
|---|---|---|---|---|
| 1 – 3 Cultivation and harvest   | 4,500 – 6,000 x g<br>4 °C, 15 min   |   |   |   |
| 4 – 5 Cell lysis<br><i>(Important:<br/>Check Buffer LYS for<br/>precipitated SDS)</i> | High-copy / low-copy<br>8 mL / 16 mL Buffer RES<br>8 mL / 16 mL Buffer LYS<br>RT, 5 min |   | High-copy / low-copy<br>12 mL / 24 mL Buffer RES<br>12 mL / 24 mL Buffer LYS<br>RT, 5 min |   |
| 6 Equilibration of the column and filter  | 12 mL<br>Buffer EQU   |  | 25 mL<br>Buffer EQU   |   |
| 7 Neutralization  | 8 mL / 16 mL Buffer NEU<br>Mix thoroughly until colorless                               |   | 12 mL / 24 mL Buffer NEU<br>Mix thoroughly until colorless                                |   |
| 8 Clarification and loading of the lysate   | Invert the tube 3 times<br>Load lysate on NucleoBond® Xtra Column Filter                |   |   |   |
| 9 1 <sup>st</sup> Wash  | 5 mL<br>Buffer EQU !  |  | 15 mL<br>Buffer EQU !   |   |
| 10 Filter removal   | Discard NucleoBond® Xtra Column Filter  |   | Discard NucleoBond® Xtra Column Filter  |   |
| 11 2 <sup>nd</sup> Wash   | 8 mL<br>Buffer WASH !   |   | 25 mL<br>Buffer WASH !  |   |
| 12 Elution  | 5 mL<br>Buffer ELU  |   | 15 mL<br>Buffer ELU   |   |
| 13 Precipitation  | <b>NucleoBond® Xtra Midi</b>  | <b>NucleoBond® Xtra Midi Plus</b>   | <b>NucleoBond® Xtra Maxi</b>  | <b>NucleoBond® Xtra Maxi Plus</b>   |
|   | 3.5 mL<br>Isopropanol<br>Vortex<br>4,5 – 15,000 x g<br>4 °C, 30 min                     | 3.5 mL<br>Isopropanol<br>Vortex<br>RT, 2 min<br>Load<br>NucleoBond®<br>Finalizer  | 10.5 mL<br>Isopropanol<br>Vortex<br>4,5 – 15,000 x g<br>4 °C, 30 min                      | 10.5 mL<br>Isopropanol<br>Vortex<br>RT, 2 min<br>Load<br>NucleoBond®<br>Finalizer Large |
| 14 Washing and drying   | 2 mL<br>70 % ethanol<br>4,5 – 15,000 x g<br>RT, 5 min<br>10 – 15 min                    | 2 mL<br>70 % ethanol<br>≥ 6 x air<br>until dry                                    | 4 mL<br>70 % ethanol<br>4,5 – 15,000 x g<br>RT, 5 min<br>15 – 30 min                      | 4 mL<br>70 % ethanol<br>≥ 6 x air until dry   |
| 15 Reconstitution   | Appropriate<br>volume of<br>TE buffer   | 200 – 800 µL<br>Buffer TRIS   | Appropriate<br>volume of<br>TE buffer   | 400 – 1000 µL<br>Buffer TRIS  |

---

## Table of contents

|      |   |    |
|------|---|----|
| 1    | Components  | 4  |
| 1.1  | Kit contents  | 4  |
| 1.2  | Reagents and equipment to be supplied by user                         | 6  |
| 2    | Kit specifications  | 7  |
| 3    | About this user manual  | 8  |
| 4    | NucleoBond® Xtra plasmid purification system                          | 9  |
| 4.1  | Basic principle   | 9  |
| 4.2  | NucleoBond® Xtra anion exchange columns                               | 9  |
| 4.3  | Growth of bacterial cultures  | 10 |
| 4.4  | Chloramphenicol amplification of low copy plasmids                    | 12 |
| 4.5  | Culture volume for high copy plasmids                                 | 12 |
| 4.6  | Culture volume for low copy plasmids                                  | 13 |
| 4.7  | Lysate neutralization and LyseControl                                 | 13 |
| 4.8  | Cell lysis  | 14 |
| 4.9  | Difficult-to-lyse strains   | 14 |
| 4.10 | Setup of NucleoBond® Xtra Columns                                     | 14 |
| 4.11 | Filtration and loading of the lysate                                  | 15 |
| 4.12 | Washing of the column   | 16 |
| 4.13 | Elution and concentration of plasmid DNA                              | 16 |
| 4.14 | Determination of DNA yield and quality                                | 19 |
| 4.15 | Convenient stopping points  | 19 |
| 5    | Storage conditions and preparation of working solutions               | 20 |
| 6    | Safety instructions   | 21 |
| 6.1  | Disposal  | 21 |
| 7    | NucleoBond® Xtra plasmid purification                                 | 22 |
| 7.1  | High copy plasmid purification (Midi, Maxi)                           | 22 |
| 7.2  | Low copy plasmid purification (Midi, Maxi)                            | 27 |
| 7.3  | Concentration of NucleoBond® Xtra eluates with NucleoBond® Finalizers | 30 |
| 8    | Appendix  | 32 |
| 8.1  | Troubleshooting   | 32 |
| 8.2  | Ordering information  | 40 |
| 8.3  | Product use restriction / warranty                                    | 42 |

# 1 Components

## 1.1 Kit contents

| REF   | NucleoBond® Xtra<br>Midi |                       |                         | NucleoBond® Xtra<br>Midi Plus |                       |
|---|--------------------------|-----------------------|-------------------------|-------------------------------|-----------------------|
|   | 10 preps<br>740410.10    | 50 preps<br>740410.50 | 100 preps<br>740410.100 | 10 preps<br>740412.10         | 50 preps<br>740412.50 |
| Buffer RES  | 100 mL                   | 500 mL                | 1000 mL                 | 100 mL                        | 500 mL                |
| Buffer LYS  | 100 mL                   | 500 mL                | 1000 mL                 | 100 mL                        | 500 mL                |
| Buffer NEU  | 100 mL                   | 500 mL                | 1000 mL                 | 100 mL                        | 500 mL                |
| Buffer EQU  | 200 mL                   | 1000 mL               | 2 x 1000 mL             | 200 mL                        | 1000 mL               |
| Buffer WASH   | 100 mL                   | 500 mL                | 1000 mL                 | 100 mL                        | 500 mL                |
| Buffer ELU  | 60 mL                    | 300 mL                | 600 mL                  | 60 mL                         | 300 mL                |
| RNase A*<br>(lyophilized)   | 6 mg                     | 30 mg                 | 60 mg                   | 6 mg                          | 30 mg                 |
| NucleoBond® Xtra<br>Midi Columns incl.<br>NucleoBond® Xtra<br>Midi Column Filters | 10                       | 50                    | 100                     | 10                            | 50                    |
| NucleoBond®<br>Finalizers   | -                        | -                     | -                       | 10                            | 50                    |
| 30 mL Syringes  | -                        | -                     | -                       | 10                            | 50                    |
| 1 mL Syringes   | -                        | -                     | -                       | 10                            | 50                    |
| Buffer TRIS   | -                        | -                     | -                       | 13 mL                         | 60 mL                 |
| Plastic Washers<br>(reusable)   | 5                        | 10                    | 10                      | 5                             | 10                    |
| User manual   | 1                        | 1                     | 1                       | 1                             | 1                     |

\* For preparation of working solutions and storage conditions see section 5.

**1.1 Kit contents *continued***

| REF   | NucleoBond® Xtra<br>Maxi |                       |                         | NucleoBond® Xtra<br>Maxi Plus |                       |
|---|--------------------------|-----------------------|-------------------------|-------------------------------|-----------------------|
|   | 10 preps<br>740414.10    | 50 preps<br>740414.50 | 100 preps<br>740414.100 | 10 preps<br>740416.10         | 50 preps<br>740416.50 |
| Buffer RES  | 150 mL                   | 750 mL                | 2 x 750 mL              | 150 mL                        | 750 mL                |
| Buffer LYS  | 150 mL                   | 750 mL                | 2 x 750 mL              | 150 mL                        | 750 mL                |
| Buffer NEU  | 150 mL                   | 750 mL                | 2 x 750 mL              | 150 mL                        | 750 mL                |
| Buffer EQU  | 500 mL                   | 2 x 1000 mL<br>500 mL | 5 x 1000 mL             | 500 mL                        | 2 x 1000 mL<br>500 mL |
| Buffer WASH   | 300 mL                   | 1000 mL<br>500 mL     | 3 x 1000 mL             | 300 mL                        | 1000 mL<br>500 mL     |
| Buffer ELU  | 180 mL                   | 900 mL                | 2 x 900 mL              | 180 mL                        | 900 mL                |
| RNase A*<br>(lyophilized)   | 10 mg                    | 50 mg                 | 2 x 50 mg               | 10 mg                         | 50 mg                 |
| NucleoBond®<br>Xtra Maxi<br>Columns incl.<br>NucleoBond®<br>Xtra Maxi Column<br>Filters | 10                       | 50                    | 100                     | 10                            | 50                    |
| NucleoBond®<br>Finalizers Large   | -                        | -                     | -                       | 10                            | 50                    |
| 30 mL Syringes  | -                        | -                     | -                       | 10                            | 50                    |
| 1 mL Syringes   | -                        | -                     | -                       | 10                            | 50                    |
| Buffer TRIS   | -                        | -                     | -                       | 13 mL                         | 60 mL                 |
| Plastic Washers<br>(reusable)   | 5                        | 10                    | 10                      | 5                             | 10                    |
| User manual   | 1                        | 1                     | 1                       | 1                             | 1                     |

\* For preparation of working solutions and storage conditions see section 5.

## 1.2 Reagents and equipment to be supplied by user

### Reagents

- Isopropanol (room-temperated)
- 70 % ethanol (room-temperated)
- Buffer for reconstitution of DNA, for example TE buffer or sterile H<sub>2</sub>O (not necessary for NucleoBond® Xtra Midi/Maxi Plus kits)

### Equipment

Standard microbiological equipment for growing and harvesting bacteria (e. g., inoculating loop, culture tubes and flasks, 37 °C shaking incubator, and centrifuge with rotor and tubes or bottles for harvesting cells)

- Refrigerated centrifuge capable of reaching  $\geq 4,500 \times g$  with rotor for the appropriate centrifuge tubes or bottles (not necessary for NucleoBond® Xtra Midi/Maxi Plus kits)
- Centrifugation tubes or vessels with suitable capacity for the volumes specified in the respective protocol
- NucleoBond® Xtra Combi Rack (see ordering information) or equivalent holder

## 2 Kit specifications

- **NucleoBond® Xtra** kits are suitable for ultra fast purification of plasmids, cosmids, and very large constructs (P1 constructs, BACs, PACs) ranging from 3 kbp up to 300 kbp. For preparation of working solutions and storage conditions see section 5.
- **NucleoBond® Xtra Columns** are polypropylene columns containing **NucleoBond® Xtra Silica Resin** packed between two inert filter elements. The columns are available in Midi and Maxi sizes with typical DNA yields of 500 µg and 1000 µg, respectively.
- All **NucleoBond® Xtra Columns** are resistant to organic solvents such as alcohol, chloroform, and phenol and are also suitable for buffers containing denaturing agents like formamide, urea, or common detergents like Triton X-100 or NP-40.
- **NucleoBond® Xtra Silica Resin** can be used over a wide pH range (pH 2.5–8.5), and can remain in contact with buffers for several hours without any change in its chromatographic properties.
- The **NucleoBond® Xtra Column Filters** are specially designed depth filters that fit into the **NucleoBond® Xtra Columns**. The filters are inserted ready-to-use in the **NucleoBond® Xtra Columns** and allow a time-saving simultaneous clearing of bacterial lysate and loading of cleared lysate onto the **NucleoBond® Xtra Column**. Furthermore, the use of the column filters avoids the time-consuming centrifugation step for lysate clearing.
- The **NucleoBond® Xtra Column Filters** allow complete removal of precipitate even with large lysate volumes without clogging and avoid shearing of large DNA constructs, such as PACs or BACs by the gentle depth filter effect.
- The **NucleoBond® Xtra Midi Plus** and **NucleoBond® Xtra Maxi Plus** kits additionally contain the **NucleoBond® Finalizers** and **NucleoBond® Finalizers Large**, respectively. These tools for a fast concentration and desalination of eluates are suitable for most plasmids and cosmids ranging from 2–50 kbp with recovery efficiencies from 40–90 % (depending on elution volume).
- **NucleoBond® Finalizer** is a polypropylene syringe filter containing a special silica membrane. The **NucleoBond® Finalizer** provides a binding capacity of 500 µg, whereas the **NucleoBond® Finalizer Large** can hold up to 2000 µg plasmid DNA.
- Due to the small dead volumes of the **NucleoBond® Finalizers** the plasmid DNA can be eluted with a concentration up to 3 µg/µL (see section 4.13, Table 4 and Table 5 for dependence of concentration on elution volume).
- All **NucleoBond® Finalizers** are resistant to organic solvents such as alcohol, chloroform, and phenol and are free of endotoxins.
- For research use only

### 3 About this user manual

All technical literature is also available on the internet at [www.mn-net.com](http://www.mn-net.com).

Please contact Technical Service regarding information about changes of the current user manual compared to previous or updated revisions.

The following section 4 provides you with a detailed description of the **NucleoBond® Xtra** purification system and important information about cell growth, cell lysis, and the subsequent purification steps. Sections 5 and 6 inform you about storage, buffer preparation, and safety instructions.

First-time users are strongly advised to read these chapters thoroughly before using this kit. Experienced users can directly proceed with the purification protocols (section 7) or just use the Protocol-at-a-glance for a quick reference.

Section 7 includes the protocols for high copy and low copy plasmid purification as well as for the concentration of **NucleoBond® Xtra** eluates with the **NucleoBond® Finalizer**. This part of the protocol is also available at [www.mn-net.com](http://www.mn-net.com) in French and German.

Each procedural step in the purification protocol is arranged like the following example taken from section 7.1:

|   | Midi        | Maxi         |
|---|-------------|--------------|
| <b>5 Cell lysis (Buffer LYS)</b>  |             |              |
| <p><b>!</b> <b>Check Lysis Buffer LYS for precipitated SDS prior to use.</b> If a white precipitate is visible, warm the buffer for several minutes at 30–40 °C until precipitate is dissolved completely. Cool buffer down to room temperature (15–25 °C).</p> <p>Add <b>Lysis Buffer LYS</b> to the suspension.</p> <p>Mix gently by <b>inverting</b> the tube <b>5 times</b>. <b>Do not vortex</b> as this will shear and release contaminating chromosomal DNA from cellular debris into the suspension.</p> <p><b>Incubate</b> the mixture at room temperature for <b>5 min</b>.</p> <p><i>Warning:</i> Prolonged exposure to alkaline conditions can irreversibly denature and degrade plasmid DNA and liberate contaminating chromosomal DNA into the lysate.</p> <p><i>Note:</i> <i>Increase LYS buffer volume proportionally if more than the recommended cell mass is used (see section 4.8 for information on optimal cell lysis).</i></p> |             |              |
|   | <b>8 mL</b> | <b>12 mL</b> |

If you are performing a Midi prep to purify plasmid DNA you will find volumes or incubation times in the white boxes. For Maxi preps please refer to the black boxes.

The name of the buffer, incubation times, repeats or important handling steps are emphasized in **bold type** within the instruction. Additional notes or optional steps are printed in *italic*. The exclamation point marks information and hints that are essential for a successful preparation.

In the example shown above you are asked to check the Lysis Buffer LYS prior to use and then to lyse the resuspended cell pellet in **8 mL** of **Buffer LYS** when performing a Midi prep and in **12 mL** for a Maxi prep. Follow the handling instructions exactly and note the given hints for protocol alterations.

## 4 NucleoBond® Xtra plasmid purification system

### 4.1 Basic principle

The bacterial cells are lysed by an optimized set of newly formulated buffers based on the NaOH/SDS lysis method of Birnboim and Doly\*.

After equilibration of the **NucleoBond® Xtra Column** together with the corresponding **NucleoBond® Xtra Column Filter**, the entire lysate is loaded by gravity flow and simultaneously cleared by the specially designed column filter.

Plasmid DNA is bound to the **NucleoBond® Xtra Silica Resin**.


After an efficient washing step the plasmid DNA is eluted, precipitated, and easily dissolved in any suitable buffer (e. g., low-salt buffer or water) for further use.

**!** **NucleoBond® Xtra Columns can not be processed by vacuum. Using NucleoBond® Xtra Columns on a vacuum manifold might lead to a complete loss of plasmid DNA.**

### 4.2 NucleoBond® Xtra anion exchange columns

**NucleoBond® Xtra** is a patented silica-based anion exchange resin, developed by MACHEREY-NAGEL. It is developed for routine separation of different classes of nucleic acids like oligonucleotides, RNA, and plasmids.

**NucleoBond® Xtra Silica Resin** consists of hydrophilic, macroporous silica beads functionalized with MAE (methyl-amino-ethanol). The dense coating of this functional group provides a high overall positive charge density under acidic pH conditions that permits the negatively charged phosphate backbone of plasmid DNA to bind with high specificity (Figure 1).

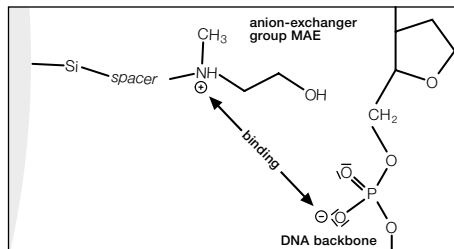


**Figure 1** Ionic interaction of the positively charged methyl-hydroxyethyl-amino group with the negative phosphate oxygen of the DNA backbone.

In contrast to the widely used DEAE (diethylaminoethyl) group, the hydroxy group of methyl-hydroxyethyl-amin can be involved in additional hydrogen bonding interactions with the DNA.

\* Birnboim, H. C. and Doly, J., (1979) Nucl. Acids Res. 7, 1513–1523

All contaminants from proteins to RNA are washed from the column, the positive charge of the resin is neutralized by a pH shift to slightly alkaline conditions, and pure plasmid DNA is eluted in a high-salt elution buffer.

The purified nucleic acid products are suitable for use in the most demanding molecular biology applications, including transfection, *in vitro* transcription, automated or manual sequencing, cloning, hybridization, and PCR.

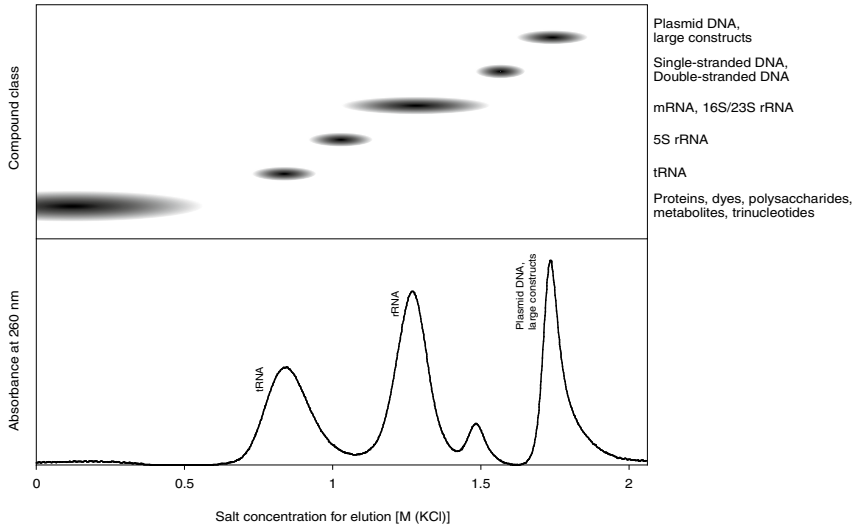

**Figure 2 Elution profile of NucleoBond® Xtra Silica Resin at pH 7.0**

The more interactions a nucleic acid can form between the phosphate backbone and the positively charged resin the later it is eluted with increasing salt concentration. Large nucleic acids carry more charges than short ones, double stranded DNA more than single stranded RNA.

### 4.3 Growth of bacterial cultures

Yield and quality of plasmid DNA highly depend on the **type of culture media** and antibiotics, the bacterial host strain, the plasmid type, size, and copy number, but also on the **growth conditions**.

For standard high copy plasmids LB (Luria-Bertani) medium is recommended. The cell culture should be incubated at 37 °C with constant shaking (200–250 rpm) preferably 12–16 h over night. Use flasks of at least three or four times the volume of the culture volume to provide a growth medium saturated with oxygen. Alternatively, rich media like 2xYT (Yeast/Tryptone), TB (Terrific Broth) or CircleGrow can be used. In this case bacteria grow faster, reach the stationary phase much earlier than in LB medium ( $\leq 2$  h), and higher cell masses can be reached. However, this does not necessarily yield more plasmid DNA. Overgrowing a culture might lead to a higher percentage of dead or starving cells and the resulting plasmid DNA might be partially degraded or contaminated with chromosomal DNA. To find the optimal culture conditions, the culture medium and incubation times have to be optimized for each host strain/plasmid construct combination individually.

Cell cultures should be grown under **antibiotic selection** at all times to ensure plasmid propagation. Without this selective pressure, cells tend to lose a plasmid during cell division. Since bacteria grow much faster without the burden of a high copy plasmid, they take over the culture rapidly and the plasmid yield goes down regardless of the cell mass. Table 1 gives information on concentrations of commonly used antibiotics.

**Table 1: Information about antibiotics according to Maniatis\***

| Antibiotic      | Stock solution (concentration) | Storage | Working concentration |
|-----------------|--------------------------------|---------|-----------------------|
| Ampicillin      | 50 mg/mL in H <sub>2</sub> O   | -20 °C  | 20–60 µg/mL           |
| Chloramphenicol | 34 mg/mL in EtOH               | -20 °C  | 25–170 µg/mL          |
| Kanamycin       | 10 mg/mL in H <sub>2</sub> O   | -20 °C  | 10–50 µg/mL           |
| Streptomycin    | 10 mg/mL in H <sub>2</sub> O   | -20 °C  | 10–50 µg/mL           |
| Tetracycline    | 5 mg/mL in EtOH                | -20 °C  | 10–50 µg/mL           |
| Carbenicillin   | 50 mg/mL in H <sub>2</sub> O   | -20 °C  | 20–60 µg/mL           |

The ***E. coli* host strain** mostly influences the quality of the plasmid DNA. Whereas strains like DH5α® or XL1-Blue usually produce high quality super-coiled plasmid DNA, other strains like for example HB101 with high levels of endonuclease activity might yield lower quality plasmid giving poor results in downstream applications like enzymatic restriction or sequencing.

The **type of plasmid**, especially the **size and the origin of replication (ori)** has a crucial influence on DNA yield. In general, the larger the plasmid or the cloned insert is, the lower is the expected DNA yield due to a lower copy number. Even a high copy construct based on a ColE1 ori can behave like a low copy vector in case of a large or unfavorable insert. In addition, the ori itself influences the yield by factor 10–100. Thus plasmids based on for example pBR322 or pACYC, cosmids or BACs are maintained at copy numbers < 20 down to even only 1, whereas vectors based on for example pUC, pBluescript or pGEM can be present in several hundred copies per cell.

Therefore, all the above mentioned factors should be taken into consideration if a particular DNA yield has to be achieved. Culture volume and lysis procedures have to be adjusted accordingly.

\* Maniatis T, Fritsch EF, Sambrook J: Molecular cloning. A laboratory manual, Cold Spring Harbor, Cold Spring, New York 1982.

## 4.4 Chloramphenicol amplification of low copy plasmids

To dramatically increase the low copy number of pMB1/colE1 derived plasmids grow the cell culture to mid or late log phase ( $OD_{600} \approx 0.6-2.0$ ) under selective conditions with an appropriate antibiotic. Then add 170  $\mu\text{g}/\text{mL}$  chloramphenicol and continue incubation for a further 8–12 hours. Chloramphenicol inhibits host protein synthesis and thus prevents replication of the host chromosome. Plasmid replication, however, is independent of newly synthesized proteins and continues for several hours until up to 2000–3000 copies per cell are accumulated\*.

Alternatively, the cell culture can be grown with only partial inhibition of protein synthesis under low chloramphenicol concentrations (10–20  $\mu\text{g}/\text{mL}$ ) resulting in a 5–10-fold greater yield of plasmid DNA\*\*.

Both methods show the positive side effect of much less genomic DNA per plasmid, but they obviously work only with plasmids that do not carry the chloramphenicol resistance gene. Furthermore, the method is only effective with low copy number plasmids under stringent control (e. g., pBR322). All modern high copy number plasmids (e. g., pUC) are already under relaxed control due to mutations in the plasmid copy number control genes and show no significant additional increase in their copy number.

## 4.5 Culture volume for high copy plasmids

Due to the influence of growth media (TB, CircleGrow, 2 xYT), growth conditions (shaking, temperature), host strain, or type of plasmid insert etc. the final amount of cells in a bacterial culture can vary over a wide range. By rule of thumb, 1 liter of *E. coli* LB culture with an  $OD_{600}$  of 1 consists of  $1 \times 10^{12}$  cells and yields about 1.5–1.8 g cell wet weight. Overnight cultures grown in LB medium usually reach an  $OD_{600}$  of 3–6 under vigorous shaking in flasks. Fermentation cultures even reach an  $OD_{600}$  of 10 and more. The expected DNA yield for a high copy plasmid is approximately 1 mg per gram cell wet weight.

It is therefore important to **adjust the cell mass rather than the culture volume** for the best plasmid purification results. But since the cell mass or cell wet weight is tedious to determine it was replaced in this manual by the mathematical product of optical density at 600 nm ( $OD_{600}$ ) and culture volume (Vol) - two variables that are much easier to measure.

$$ODV = OD_{600} \times Vol \text{ [mL]}$$

Note that for a correct OD determination the culture samples have to be diluted if  $OD_{600}$  exceeds 0.5 in order to increase proportionally with cell mass. For a well grown *E. coli* culture a 1:10 dilution with fresh culture medium is recommended. The measured  $OD_{600}$  is then multiplied with the dilution factor 10 to result in a theoretical  $OD_{600}$  value. This  $OD_{600}$  is used in Table 2 to determine the appropriate culture volume. Table 2 shows recommended ODVs and the corresponding pairs of  $OD_{600}$  and culture volume that can be easily handled using the standard kit protocol lysis buffer volumes. For example, if the  $OD_{600}$  of your *E. coli* culture is 6, use 66 mL culture for a Midi prep or 200 mL for a Maxi prep.

---

\* Maniatis T, Fritsch EF, Sambrook J: Molecular cloning. A laboratory manual, Cold Spring Harbor, Cold Spring, New York 1982.

\*\* Frenkel L, Bremer H: Increased amplification of plasmids pBR322 and pBR327 by low concentrations of chloramphenicol, DNA (5), 539 – 544, 1986..

**Table 2: Recommended culture volumes for high copy plasmids**

| NucleoBond® Xtra | Pellet wet weight | Rec. ODV | OD <sub>600</sub> = 2 | OD <sub>600</sub> = 4 | OD <sub>600</sub> = 6 | OD <sub>600</sub> = 8 | OD <sub>600</sub> = 10 |
|------------------|-------------------|----------|-----------------------|-----------------------|-----------------------|-----------------------|------------------------|
| Midi             | 0.75 g            | 400      | 200 mL                | 100 mL                | 66 mL                 | 50 mL                 | 40 mL                  |
| Maxi             | 2.25 g            | 1200     | 600 mL                | 300 mL                | 200 mL                | 150 mL                | 120 mL                 |

## 4.6 Culture volume for low copy plasmids

**NucleoBond® Xtra** kits are designed for isolation of high copy plasmids (up to several hundred copies/cell) as well as low copy plasmids (< 20 copies/cell). However, when purifying low copy plasmids, the cell mass and the lysis buffer volumes should be increased at least by factor 2 to provide enough DNA to utilize the columns' binding capacity. Table 3 shows recommended ODVs and the corresponding pairs of OD<sub>600</sub> and culture volume for low copy plasmid cell cultures (for detailed information on calculating ODV = OD<sub>600</sub> × Vol. refer to section 4.5). For example, if the OD<sub>600</sub> of your *E. coli* culture is 6, use 133 mL culture for a Midi prep or 400 mL for a Maxi prep.

**Table 3: Recommended culture volumes for low copy plasmids**

| NucleoBond® Xtra | Pellet wet weight | Rec. ODV | OD <sub>600</sub> = 2 | OD <sub>600</sub> = 4 | OD <sub>600</sub> = 6 | OD <sub>600</sub> = 8 | OD <sub>600</sub> = 10 |
|------------------|-------------------|----------|-----------------------|-----------------------|-----------------------|-----------------------|------------------------|
| Midi             | 1.5 g             | 800      | 400 mL                | 200 mL                | 133 mL                | 100 mL                | 80 mL                  |
| Maxi             | 4.5 g             | 2400     | 1200 mL               | 600 mL                | 400 mL                | 300 mL                | 240 mL                 |

For higher yields, it is advantageous to increase the cell culture and lysis buffer volumes even more (e. g., by factor 3–5). In this case additional lysis buffer can be ordered separately (see ordering information). Furthermore, a centrifuge should be used for lysate clarification instead of the provided **NucleoBond® Xtra Column Filters** since their capacity for precipitate is limited.

Alternatively, chloramphenicol amplification can be considered to increase the plasmid copy number (see section 4.4)

## 4.7 Lysate neutralization and LyseControl

Proper mixing of the lysate with Neutralization Buffer NEU is of utmost importance for complete precipitation of SDS, protein, and genomic DNA. Incomplete neutralization leads to reduced yields, slower flow-rates, and potential clogging of the **NucleoBond® Xtra** Column Filter. However, released plasmid DNA is very vulnerable at this point and shaking too much or too strongly will damage the DNA.

Therefore, **do not vortex or shake** but **just invert the mixture very gently** until a fluffy off-white precipitate has formed and the **LyseControl** has turned **colorless** throughout the lysate without any traces of blue color.

## 4.8 Cell lysis

The bacterial cell pellet is resuspended in Buffer RES and lysed by a sodium hydroxide/SDS treatment with Buffer LYS. Proteins, as well as chromosomal and plasmid DNA are denatured under these conditions. RNA is degraded by RNase A. Neutralization Buffer NEU, containing potassium acetate, is then added to the lysate, causing SDS to precipitate as KDS (potassium dodecyl sulfate) and pulling down proteins, chromosomal DNA, and other cellular debris. The potassium acetate buffer also neutralizes the lysate. Plasmid DNA can revert to its native supercoiled structure and remains in solution.

The **NucleoBond® Xtra** buffer volumes (standard protocol) are adjusted to ensure optimal lysis for culture volumes, appropriate for high copy plasmids according to section 4.5, Table 2. Using too much cell material leads to inefficient cell lysis and precipitation and might reduce plasmid yield and purity. Therefore, lysis buffer volumes should be increased when applying larger culture volumes in case of for example low copy vector purification (section 4.6, Table 3).

**By rule of thumb, calculate the necessary lysis buffer volumes for RES, LYS, and NEU as follows:**

$$\text{Vol. [mL]} = \text{Culture Volume [mL]} \times \text{OD}_{600} / 50$$

For example, if 200 mL of a low copy bacterial culture ( $\text{OD}_{600} = 4$ ) is to be lysed, the appropriate volumes of lysis buffers RES, LYS, and NEU are 16 mL each. If more lysis buffer is needed than is provided with the kit, an additional buffer set including buffers RES, LYS, NEU, and RNase A can be ordered separately (see ordering information).

By using sufficient amounts of lysis buffer, lysis time can be limited to 3–4 minutes and should not exceed 5 minutes. Prolonged exposure to alkaline conditions can irreversibly denature and degrade plasmid DNA and liberate contaminating chromosomal DNA into the lysate.


Please note that the calculated lysis buffer volumes for **NucleoBond® Xtra Maxi** preparations do not match the recommended volumes in the protocol due to the fact that most users start with much less cells than the recommended ODV 1200. Furthermore, the 3 x 12 mL of the protocol can conveniently be used in combination with 50 mL centrifugation tubes. More lysis buffer usually requires to split the sample.

## 4.9 Difficult-to-lyse strains

For plasmid purification of for example Gram-positive bacteria or strains with a more resistant cell wall it might be advantageous to start the preparation with a lysozyme treatment. Therefore, resuspend the cell pellet in Buffer RES containing **2 mg/mL lysozyme** and incubate at **37 °C for 30 minutes**. Proceed then with the lysis procedure according to the **NucleoBond® Xtra** standard protocol.

## 4.10 Setup of NucleoBond® Xtra Columns

Ideally the **NucleoBond® Xtra Midi** or **Maxi Columns** are placed into a **NucleoBond® Xtra Combi Rack** (see ordering information). They are held either by the collar ring of the cartridges or by the Plastic Washers (reusable) included in the kit to individually adjust the height of each column (see Figure 3). The Plastic Washers (reusable) can also be used to hold the columns on top of suitable collection tubes or flasks. The **NucleoBond® Xtra Combi Rack** can be used in combination with **NucleoBond® PC 100, 500, and 2000** as well. Note that the **NucleoBond® Xtra Midi Columns** can also be placed in the **NucleoBond® Rack Large** (REF 740563).

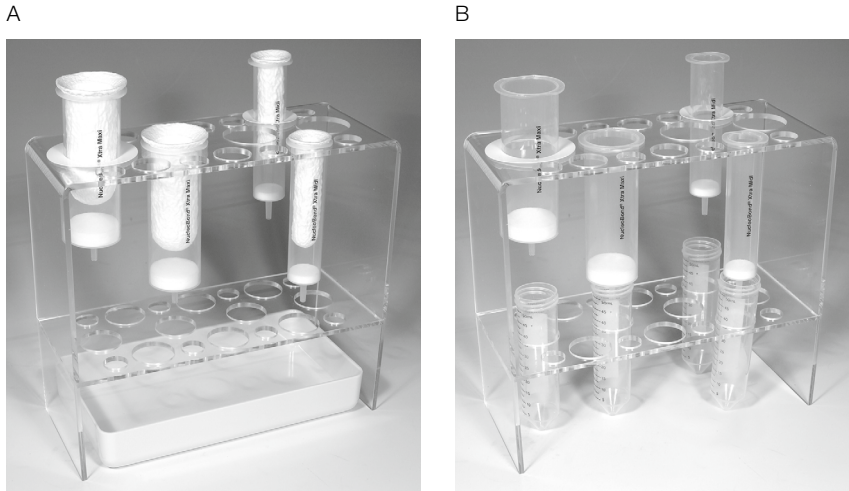


**Figure 3 Setup of NucleoBond® Xtra Midi / Maxi Columns with the NucleoBond® Xtra Combi Rack**

A: Setup for clarification, loading, and first washing step; B: Setup for elution.

## 4.11 Filtration and loading of the lysate

After the alkaline lysis, the sample has to be cleared from cell debris and precipitate to ensure high plasmid purity and a fast column flow rate. This is achieved by passing the solution through a **NucleoBond® Xtra Column Filter** which is provided already inserted into the **NucleoBond® Xtra Column**.

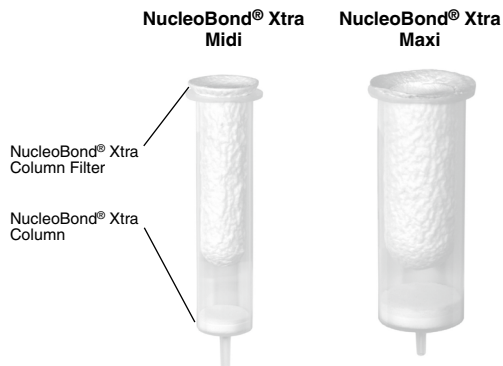

The **NucleoBond® Xtra Column Filters** are designed to eliminate the centrifugation step after alkaline lysis. They are pre-wet during column equilibration and allow a time-saving simultaneous clearing of bacterial lysate and loading of the **NucleoBond® Xtra Column**.

Compared to lysate clearing by centrifugation or syringe filters the **NucleoBond® Xtra Column Filter** furthermore avoids shearing of large DNA constructs such as PACs or BACs by the gentle depth filter effect (filtration occurs on the surface of the filter as well as inside the filter matrix). Its special material and design lead to very rapid passage of the lysate through the filter and even very large lysate volumes can be applied without the risk of clogging. This is especially important for low copy plasmid purification for example. However, if more than the recommended cell mass (see section 4.5, Table 2, section 4.6, Table 3) was lysed, it might be advantageous to use a centrifuge for lysate clarification rather than the provided column filters due to their limited precipitate capacity.

## 4.12 Washing of the column

The high salt concentration of the lysate prevents proteins and RNA from binding to the **NucleoBond® Xtra Column** (see section 4.2, Figure 2). However, to remove all traces of contaminants and to purge the dead volume of the **NucleoBond® Xtra Column Filters** it is important to wash the column and the filter in two subsequent washing steps.

First apply **Equilibration Buffer EQU** to the funnel rim of the filter to wash all residual lysate out of the filter onto the column. Do not just pour the buffer inside the filter. Then pull out and discard the column filter or remove the filter by turning the column upside down. It is essential to wash the **NucleoBond® Xtra Column** without filter for a second time with **Wash Buffer WASH**. This ensures highest yields with best achievable purity.

## 4.13 Elution and concentration of plasmid DNA

Elution is carried out under high-salt conditions and by a shift of pH from 7.0 to 9.0. Under these alkaline conditions the positive charge of the anion exchange resin is neutralized and plasmid DNA is released. For any downstream application it is necessary to precipitate the DNA and to remove salt and all traces of alcohol since they disturb or inhibit enzymatic activity needed for restriction or sequencing reactions.

All **NucleoBond® Xtra** eluates already contain enough salt for an isopropanol precipitation of DNA. Therefore the precipitation is started by directly adding 0.7 volumes of isopropanol. To prevent co-precipitation of salt, use **room-temperature isopropanol** only and do not let the plasmid DNA solution drop into a vial with isopropanol but **add isopropanol to the final eluate and mix immediately**.

Afterwards either follow the centrifugation protocol given after the **NucleoBond® Xtra** purification protocol or follow the support protocol for the **NucleoBond® Finalizers** in section 7.3 to eliminate the time-consuming centrifugation steps for precipitation (use of **NucleoBond® Finalizers** is only recommended for vector sizes smaller than 50 kbp).


The **NucleoBond® Finalizers** are designed for quick concentration and desalination of plasmid and cosmid DNA eluates that are obtained by anion exchange chromatography based DNA purification. The sample is precipitated with isopropanol as mentioned above and loaded onto a special silica membrane by means of a syringe. After an ethanolic washing step the membrane is dried by pressing air through the filter. Elution of pure DNA is carried out with slightly alkaline low salt buffers like **Buffer TRIS** (5 mM Tris/HCl, pH 8.5, provided with all **NucleoBond® Xtra Plus** kits) or TE buffer (10 mM Tris/HCl, pH 7.5, 1 mM EDTA). Do not use pure water unless pH is definitely higher than 7.0

**For maximum yield it is recommended to perform the elution step twice.** The first elution step is done using fresh buffer whereas in the second elution step the eluate from the first elution is reapplied on the **NucleoBond® Finalizer** to allow complete solubilization of the plasmid.

**DNA recovery highly depends on the used elution buffer volume.** Large volumes result in a high recovery of up to 90 % but in a lower DNA concentration. Small elution volumes on the other hand increase the concentration but at the cost of DNA yield.

If a small volume is chosen, make sure to recover as much eluate as possible from the syringe and **NucleoBond® Finalizer** by pressing air through the **NucleoBond® Finalizer** several times after elution and collecting every single droplet to minimize the dead volume.

Figure 4 and Figure 5 illustrate exemplarily how DNA recovery and final DNA concentration depend on the buffer volume which is used for elution of DNA from the **NucleoBond® Finalizer** and **NucleoBond® Finalizer Large**, respectively.

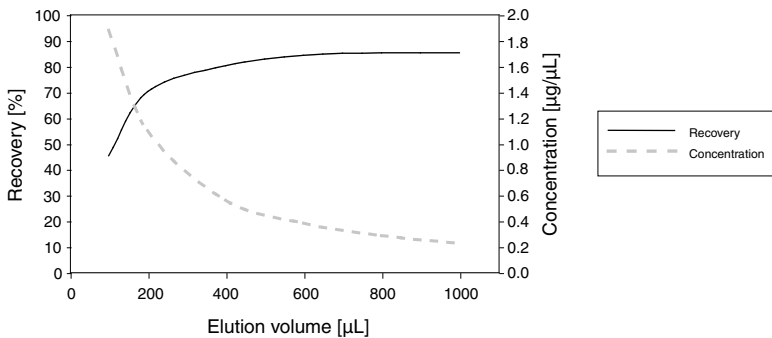

**Figure 4 Final DNA recovery and concentration after NucleoBond® Finalizer application**

A NucleoBond® Xtra Midi eluate containing 250 µg plasmid DNA (8 kbp) was loaded onto a NucleoBond® Finalizer and eluted two-fold with increasing volumes of TE buffer.

The **NucleoBond® Finalizer** is designed to hold a maximum of 500 µg DNA and is therefore ideally suited to be used in combination with **NucleoBond® Xtra Midi**. Maximum DNA recovery can be achieved by using > 600 µL of elution buffer. For a higher concentration experienced users can lower the elution buffer volume to 400–200 µL.

Table 4 gives an overview about recovery and concentration of different amounts of plasmid DNA loaded onto a **NucleoBond® Finalizer**. DNA was eluted two-fold with increasing volumes of TE. Please refer to this tables to select an elution buffer volume that meets your needs best.

Table 4: DNA recovery and concentration for the NucleoBond® Finalizer

|            |           | Elution volume |           |           |           |             |           |
|------------|-----------|----------------|-----------|-----------|-----------|-------------|-----------|
|            |           | 100 µL         | 200 µL    | 400 µL    | 600 µL    | 800 µL      | 1000 µL   |
| Loaded DNA | 500 µg    | 35 %           | 60 %      | 70 %      | 75 %      | 75 %        | 75 %      |
|            |           | 2.5 µg/µL      | 2.3 µg/µL | 1.2 µg/µL | 0.8 µg/µL | 0.6 µg/µL   | 0.5 µg/µL |
|            | 250 µg    | 40 %           | 65 %      | 75 %      | 80 %      | 80 %        | 80 %      |
|            |           | 1.9 µg/µL      | 1.1 µg/µL | 0.6 µg/µL | 0.4 µg/µL | 0.3 µg/µL   | 0.2 µg/µL |
|            | 100 µg    | 45 %           | 70 %      | 80 %      | 85 %      | 85 %        | 85 %      |
|            |           | 0.7 µg/µL      | 0.4 µg/µL | 0.2 µg/µL | 0.1 µg/µL | 0.1 µg/µL   | 0.1 µg/µL |
| 50 µg      | 30 %      | 75 %           | 85 %      | 90 %      | 90 %      | 90 %        |           |
|            | 0.3 µg/µL | 0.2 µg/µL      | 0.1 µg/µL | 0.1 µg/µL | 0.1 µg/µL | < 0.1 µg/µL |           |

|                   |
|-------------------|
| DNA recovery      |
| DNA concentration |

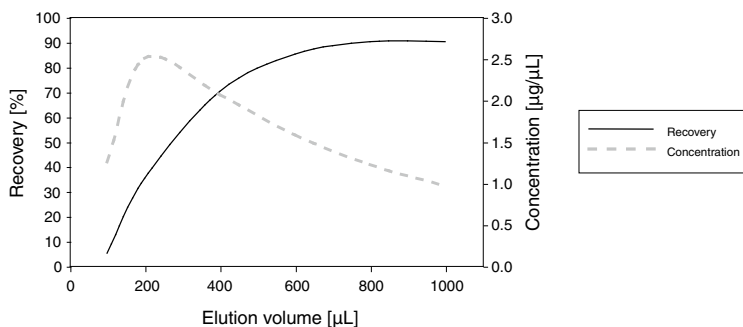


Figure 5 Final DNA recovery and concentration after NucleoBond® Finalizer Large application

A NucleoBond® Xtra Maxi eluate containing 1000 µg plasmid DNA (8 kbp) was loaded onto a NucleoBond® Finalizer Large and eluted two-fold with increasing volumes of TE buffer.

NucleoBond® Xtra Maxi eluates are easily concentrated with a NucleoBond® Finalizer Large which is able to bind up to 2000 µg plasmid DNA. Maximum DNA recovery can be achieved by using > 800 µL of elution buffer. For a higher concentration experienced users can lower the elution buffer volume to 600–400 µL.

Table 5 gives an overview about recovery and concentration of different amounts of plasmid DNA loaded onto a NucleoBond® Finalizer Large. DNA was eluted two-fold with increasing volumes of TE. Please refer to this tables to select an elution buffer volume that meets your needs best.

Table 5: DNA recovery and concentration for the NucleoBond® Finalizer Large

|            | Elution volume |           |           |           |           |           |           |
|------------|----------------|-----------|-----------|-----------|-----------|-----------|-----------|
|            | 100 µL         | 200 µL    | 400 µL    | 600 µL    | 800 µL    | 1000 µL   |           |
| Loaded DNA | 1500 µg        | 5 %       | 30 %      | 65 %      | 80 %      | 85 %      | 90 %      |
|            |                | 1.9 µg/µL | 3.2 µg/µL | 2.9 µg/µL | 2.2 µg/µL | 1.7 µg/µL | 1.4 µg/µL |
|            | 1000 µg        | 5 %       | 35 %      | 70 %      | 85 %      | 90 %      | 90 %      |
|            |                | 1.3 µg/µL | 2.5 µg/µL | 2.1 µg/µL | 1.6 µg/µL | 1.2 µg/µL | 1.0 µg/µL |
|            | 500 µg         | 10 %      | 40 %      | 70 %      | 85 %      | 90 %      | 90 %      |
|            |                | 1.3 µg/µL | 1.4 µg/µL | 1.0 µg/µL | 0.8 µg/µL | 0.6 µg/µL | 0.5 µg/µL |
| 100 µg     | 15 %           | 45 %      | 70 %      | 80 %      | 85 %      | 90 %      |           |
|            | 0.4 µg/µL      | 0.3 µg/µL | 0.2 µg/µL | 0.1 µg/µL | 0.1 µg/µL | 0.1 µg/µL |           |

|                   |
|-------------------|
| DNA recovery      |
| DNA concentration |

#### 4.14 Determination of DNA yield and quality

The **yield** of a plasmid preparation should be estimated prior to and after the isopropanol precipitation in order to calculate the recovery after precipitation and to find the best volume to dissolve the pellet in. Simply use either **NucleoBond® Xtra** Elution Buffer ELU or the respective low-salt buffer as a blank in your photometric measurement.

The nucleic acid **concentration** of the sample can be calculated from its UV absorbance at 260 nm where an absorbance of 1 (1 cm path length) is equivalent to 50 µg DNA/mL. Note that the absolute measured absorbance should lie between 0.1 and 0.7 in order to be in the linear part of Lambert-Beer's law. Dilute your sample in the respective buffer if necessary.

The plasmid **purity** can be checked by UV spectroscopy as well. A ratio of  $A_{260}/A_{280}$  between 1.80 – 1.90 and  $A_{260}/A_{230}$  around 2.0 indicates pure plasmid DNA. An  $A_{260}/A_{280}$  ratio above 2.0 is a sign for too much RNA in your preparation, an  $A_{260}/A_{280}$  ratio below 1.8 indicates protein contamination.

Plasmid **quality** can be checked by running the precipitated samples on a 1 % agarose gel. This will give information on conformation and structural integrity of isolated plasmid DNA, i. e. it shows whether the sample is predominantly present in the favorable super-coiled form (ccc, usually the fastest band), as an open circle (oc), or even in a linear form (see section 8.1, Figure 6).

#### 4.15 Convenient stopping points

Cell pellets can easily be stored for several months at -20 °C.

Cleared lysates can be kept on ice or at 4 °C for several days.

For optimal performance the column purification should not be interrupted. However, the columns can be left unattended for several hours since the columns do not run dry. This might cause only small losses in DNA yield.

The eluate can be stored for several days at 4 °C. Note that the eluate should be warmed up to room temperature before precipitating the DNA to avoid co-precipitation of salt.

## 5 Storage conditions and preparation of working solutions

All kit components can be stored at 15–25 °C and are stable until: see Package label.

Storage of Buffer LYS below 20 °C may cause precipitation of SDS. If salt precipitate is observed, incubate buffer at 30–40 °C for several minutes and mix well until all precipitate is redissolved completely. Cool down to room temperature before use.

Before the first use of the **NucleoBond® Xtra Midi/Maxi** kit, prepare the following:

- Dissolve the lyophilized RNase A\* by the addition of 1 mL of Buffer RES. Wearing gloves is recommended. Pipette up and down until the RNase A is dissolved completely. Transfer the RNase A solution back to the bottle containing Buffer RES and shake well. Note the date of RNase A addition. The final concentration of RNase A is 60 µg/mL Buffer RES. Store Buffer RES with RNase A at 4 °C. The solution will be stable at this temperature for at least 6 months.

---

\* REF 740414.100 contains 2 x 50 mg of RNase A. Make sure to dissolve RNase A of both vials, each in 1 mL of Buffer RES, and transfer the solution back into the bottle containing Buffer RES.

## 6 Safety instructions

When working with the **NucleoBond® Xtra** kit wear suitable protective clothing (e.g., lab coat, disposable gloves, and protective goggles). For more information consult the appropriate Material Safety Data Sheets (MSDS available online at <http://www.mn-net.com/msds>).



The waste generated with the **NucleoBond® Xtra** kit has not been tested for residual infectious material. A contamination of the liquid waste with residual infectious material is highly unlikely due to strong denaturing lysis buffer treatment but it cannot be excluded completely. Therefore, liquid waste must be considered infectious and should be handled and discarded according to local safety regulations.

### 6.1 Disposal

Dispose hazardous, infectious or biologically contaminated materials in a safe and acceptable manner and in accordance with all local and regulatory requirements.

## 7 NucleoBond® Xtra plasmid purification

The following section includes the protocols for high copy and low copy plasmid purification as well as for concentration of NucleoBond® Xtra eluates with the NucleoBond® Finalizers.

### 7.1 High copy plasmid purification (Midi, Maxi)

|   | Midi   | Maxi                               |
|---|--|------------------------------------|
| <b>1 Preparation of starter culture</b>         |  |                                    |
|   | Inoculate a 3–5 mL starter culture of LB medium with a single colony picked from a freshly streaked agar plate. Make sure that plate and liquid culture contain the appropriate selective antibiotic to guarantee plasmid propagation (see section 4.3 for more information). Shake at 37 °C and ~ 300 rpm for ~ 8 h.  |                                    |
| <b>2 Preparation of large overnight culture</b> |  |                                    |
|   | Inoculate an overnight culture by diluting the starter culture 1/1000 into the given volumes of LB medium also containing the appropriate selective antibiotic. Grow the culture overnight at 37 °C and ~ 300 rpm for 12–16 h.   |                                    |
|   | 100 mL   | 300 mL                             |
| <b>3 Harvest of bacterial cells</b>             |  |                                    |
|   | Measure the cell culture $OD_{600}$ and determine the recommended culture volume.  |                                    |
|   | $V \text{ [mL]} = 400 / OD_{600}$  | $V \text{ [mL]} = 1200 / OD_{600}$ |
|   | Pellet the cells by centrifugation at <b>4,500–6,000 x g</b> for <b>≥ 10 min</b> at <b>4 °C</b> and discard the supernatant completely.  |                                    |
|   | <i>Note: Optimal lysis conditions are achieved by a unique ratio of lysis buffer RES, LYS, and NEU to the cell mass. See section 4.5 for recommendations concerning the optimal pelleted culture volume for cells containing high copy plasmids and section 4.6 for recommendations concerning cells with low copy plasmids. Read section 4.5 carefully as excess cell input will result in reduced yield. The recommended culture volumes below are calculated for a final <math>OD_{600}</math> of around 4.</i> |                                    |
| <b>4 Resuspension (Buffer RES)</b>              |  |                                    |
|   | Resuspend the cell pellet completely in <b>Resuspension Buffer RES + RNase A</b> by pipetting the cells up and down or vortexing the cells.  |                                    |
|   | For an efficient cell lysis it is important that no clumps remain in the suspension.   |                                    |
|   | <i>Note: Increase RES buffer volume proportionally if more than the recommended cell mass is used (see section 4.8 for information on optimal cell lysis and section 4.9 regarding difficult-to-lyse strains).</i>   |                                    |
|   | 8 mL   | 12 mL                              |

Midi

Maxi

**5 Cell lysis (Buffer LYS)**

- !** Check Lysis Buffer LYS for precipitated SDS prior to use. If a white precipitate is visible, warm the buffer for several minutes at 30–40 °C until precipitate is dissolved completely. Cool buffer down to room temperature.

Add **Lysis Buffer LYS** to the suspension.

Mix gently by **inverting** the tube **5 times**. **Do not vortex** as this will shear and release contaminating chromosomal DNA from cellular debris into the suspension.

**Incubate** the mixture at room temperature for **5 min**.

Warning: Prolonged exposure to alkaline conditions can irreversibly denature and degrade plasmid DNA and liberate contaminating chromosomal DNA into the lysate.

Note: Increase LYS buffer volume proportionally if more than the recommended cell mass is used (see section 4.8 for information on optimal cell lysis).

8 mL


12 mL

**6 Equilibration (Buffer EQU)**

Equilibrate a **NucleoBond® Xtra Column** together with the inserted column filter with **Equilibration Buffer EQU**.

Apply the buffer onto the rim of the column filter as shown in the picture and make sure to wet the entire filter.

Allow the column to empty by gravity flow. The column does not run dry.



12 mL

25 mL

Midi

Maxi

## 7 Neutralization (Buffer NEU)

- ! Add **Neutralization Buffer NEU** to the suspension and immediately mix the lysate gently by **inverting** the tube **until blue samples turns colorless completely!** Do not vortex.

The flask or tube used for this step should not be filled more than two thirds to allow homogeneous mixing. Make sure to neutralize completely to precipitate all the protein and chromosomal DNA. The lysate should turn from a slimy, viscous consistency to a low viscosity, homogeneous suspension of an off-white flocculate. In addition, LyseControl should turn completely colorless without any traces of blue.

Immediately proceed with step 8. **An incubation of the lysate is not necessary.**

*Note:* Increase NEU buffer volume proportionally if more than the recommended cell mass is used (see section 4.8 for information on optimal cell lysis).

*Optional:* Pre-chill Neutralisation Buffer NEU on ice before addition or refrigerate prior to use.

8 mL

12 mL

## 8 Clarification and loading

- ! Make sure to have a homogeneous suspension of the precipitate by **inverting the tube 3 times** directly before applying the lysate to the equilibrated NucleoBond® Xtra Column Filter to avoid clogging of the filter.

The lysate is simultaneously cleared and loaded onto the column. Refill the filter if more lysate has to be loaded than the filter is able to hold. Allow the column to empty by gravity flow.




*Optional:* Incubate crude lysate for 5 minutes on ice prior to loading.

*Note:* The lysate appears turbid after passing the filter. The turbidity is not caused by precipitate passing the filter, it does not clog the column, it rather indicates correct working of the procedure.

**Alternative:** The precipitate can be removed by centrifugation at  $\geq 5,000 \times g$  for at least 10 min, for example if more than double the recommended cell mass was used. If the supernatant still contains suspended matter transfer it to a new tube and repeat the centrifugation, preferably at higher speed, or apply the lysate to the equilibrated NucleoBond® Xtra Column Filter.

This clarification step is extremely important since residual precipitate may clog the NucleoBond® Xtra Column. To load the column you can either apply the cleared lysate to the equilibrated filter or remove the unused filter beforehand. Allow the column to empty by gravity flow.

*Note:* You may want to save all or part of the flow-through for analysis (see section 8.1).

|  | Midi  | Maxi  |
|--|---|-------|
| <b>9 1<sup>st</sup> Wash: Column filter and column (Buffer EQU)</b>  |   |       |
| <p>! Wash the NucleoBond® Xtra Column Filter and <b>NucleoBond® Xtra</b> Column with <b>Equilibration Buffer EQU</b>.</p> <p>Apply the buffer to the funnel shaped rim of the filter and make sure it is washing out the lysate which is remaining in the filter. Omitting this step or just pouring the buffer directly inside the funnel may reduce plasmid yield.</p>   |  |       |
|  | 5 mL  | 15 mL |
| <b>10 Filter removal</b>   |   |       |
| <p>Either pull out the NucleoBond® Xtra Column Filter or discard it by turning the column upside down.</p>   |  |       |
| <b>11 2<sup>nd</sup> Wash: Column only (Buffer WASH)</b>   |   |       |
| <p>! Wash the NucleoBond® Xtra Column with <b>Wash Buffer WASH</b>. It is important to remove the column filter before applying the washing buffer to avoid low purity.</p>  |  |       |
|  | 8 mL  | 25 mL |
| <b>12 Elution (Buffer ELU)</b>   |   |       |
| <p>Elute the plasmid DNA with <b>Elution Buffer ELU</b>. Collect the eluate in a 15 mL or 50 mL centrifuge tube (not provided).</p> <p><i>Note:</i> Preheating Buffer ELU to 50 °C prior to elution may improve yields for large constructs such as BACs.</p> <p><i>Optional:</i> Determine plasmid yield by UV spectrophotometry in order to adjust desired concentration of DNA in step 15 and calculate the recovery after precipitation.</p> |   |       |
|  | 5 mL  | 15 mL |
| <p>! <b>NucleoBond® Xtra Midi / Maxi Plus:</b></p> <p>Proceed with <b>step 13</b> for the centrifugation protocol after isopropanol precipitation or continue with <b>section 7.3</b> for plasmid concentration and desalting by using the NucleoBond® Finalizer (NucleoBond® Xtra Midi Plus) or NucleoBond® Finalizer Large (NucleoBond® Xtra Maxi Plus).</p>   |   |       |

Midi

Maxi

**13 Precipitation**

Add **room-temperature isopropanol** to precipitate the eluted plasmid DNA.

**Vortex thoroughly!**

Centrifuge at  $\geq 4,500 \times g$  for  $\geq 15$  min at  $\leq$  **room temperature**, preferably at  $15,000 \times g$  for **30 min** at **4 °C**. Carefully discard the supernatant.

3.5 mL

10.5 mL

**14 Washing and drying**

Add **room-temperature 70 % ethanol** to the pellet.

2 mL

4 mL

Centrifuge at  $\geq 4,500 \times g$ , preferably  $\geq 15,000 \times g$  for **5 min** at **room temperature**.

Carefully remove ethanol completely from the tube with a pipette tip. Allow the pellet to dry at **room temperature**.

*Note: Plasmid DNA might be harder to dissolve when over-dried.*

10–15 min

15–30 min

**15 Reconstitution**

Dissolve the DNA pellet in an appropriate volume of buffer TE or sterile H<sub>2</sub>O. Depending on the type of centrifugation tube, dissolve under gentle pipetting up and down or constant spinning in a sufficient amount of buffer for 10–60 min (3D-shaker).

Determine plasmid yield by UV spectrophotometry. Confirm plasmid integrity by agarose gel electrophoresis (see section 4.14).

## 7.2 Low copy plasmid purification (Midi, Maxi)

The lysis buffer volumes provided in the kit are adjusted for high copy plasmid purification. Therefore, additional buffer has to be ordered separately for routine purification of low copy plasmids (see ordering information).

|   | Midi   | Maxi   |
|---|--|--------|
| <b>1 Preparation of starter culture</b>         |  |        |
|   | Inoculate a 3–5 mL starter culture of LB medium with a single colony picked from a freshly streaked agar plate. Make sure that plate and liquid culture contain the appropriate selective antibiotic to guarantee plasmid propagation (see section 4.3 for more information). Shake at 37 °C and ~ 300 rpm for ~ 8 h.  |        |
| <b>2 Preparation of large overnight culture</b> |  |        |
|   | <p><b>!</b> <i>Note:</i> To utilize the entire large binding capacity of the NucleoBond® Xtra Columns it is important to provide enough plasmid DNA. For the standard low copy procedure the culture volumes were doubled compared to the high copy vector protocol. However, due to a plasmid content that is 10–100 times lower, this might be insufficient. If you need large amounts of low copy plasmids, <b>further increase the culture volume by factor 3–5. The recommended culture volumes below are calculated for a final OD<sub>600</sub> of around 4 (see section 4.6 for more information).</b></p> |        |
|   | Inoculate an overnight culture by diluting the starter culture 1/1000 into the given volumes of LB medium also containing the appropriate selective antibiotic. Grow the culture overnight at 37 °C and ~ 300 rpm for 12–16 h.   |        |
|   | 200 mL   | 600 mL |

### 3 Harvest of bacterial cells

Measure the cell culture OD<sub>600</sub> and determine the recommended culture volume.

|                                   |                                    |
|-----------------------------------|------------------------------------|
| $V \text{ [mL]} = 800 / OD_{600}$ | $V \text{ [mL]} = 2400 / OD_{600}$ |
|-----------------------------------|------------------------------------|

Pellet the cells by centrifugation at **4,500–6,000 x g** for **≥ 10 min** at **4 °C** and discard the supernatant completely.

*Note:* It is of course possible to use larger culture volumes, for example if a large amount of low copy plasmid is needed (see section 4.6 for more information). In this case increase RES, LYS and NEU buffer volumes proportionally in steps 4, 5 and 7. **Additional lysis buffer volumes might have to be ordered separately (see ordering information for NucleoBond® Xtra Buffer Set I, section 8.2).** Use a centrifuge for the lysate clarification rather than the NucleoBond® Xtra Column Filters.

Midi

Maxi

**4 Resuspension (Buffer RES)**

Resuspend the cell pellet completely in **Resuspension Buffer RES + RNase A** by pipetting the cells up and down or vortexing the cells.

For an efficient cell lysis it is important that no clumps remain in the suspension.

*Note: Increase RES buffer volume proportionally if more than the recommended cell mass is used (see section 4.8 for information on optimal cell lysis and section 4.9 regarding difficult-to-lyse strains).*

16 mL

24 mL

**5 Cell lysis (Buffer LYS)**

**Check Lysis Buffer LYS for precipitated SDS prior to use.** If a white precipitate is visible, warm the buffer for several minutes at 30–40 °C until precipitate is dissolved completely. Cool buffer down to room temperature.

Add **Lysis Buffer LYS** to the suspension.

*Note: Increase LYS buffer volume proportionally if more than the recommended cell mass is used (see section 4.8 for information on optimal cell lysis).*

16 mL

24 mL

Mix gently by **inverting** the tube **5 times**. **Do not vortex** as this will shear and release contaminating chromosomal DNA from cellular debris into the suspension.

**Incubate** the mixture at room temperature for **5 min**.


**Warning:** Prolonged exposure to alkaline conditions can irreversibly denature and degrade plasmid DNA and liberate contaminating chromosomal DNA into the lysate.

**6 Equilibration (Buffer EQU)**

Equilibrate a NucleoBond® Xtra Column together with the inserted column filter with **Equilibration Buffer EQU**.

Apply the buffer onto the rim of the column filter as shown in the picture and make sure to wet the entire filter.

Allow the column to empty by gravity flow. The column does not run dry.



12 mL

25 mL

Midi

Maxi

**7 Neutralization (Buffer NEU)**

Add **Neutralization Buffer NEU** to the suspension and immediately mix the lysate gently by **inverting** the tube **until blue samples turns colorless completely! Do not vortex.**

**!**

The flask or tube used for this step should not be filled more than two thirds to allow homogeneous mixing. Make sure to neutralize completely to precipitate all the protein and chromosomal DNA. The lysate should turn from a slimy, viscous consistency to a low viscosity, homogeneous suspension of an off-white flocculate. In addition, LyseControl should turn completely colorless without any traces of blue.

*Note: Increase NEU buffer volume proportionally if more than the recommended cell mass is used (see section 4.8 for information on optimal cell lysis).*

*Optional: Pre-chill Neutralisation Buffer NEU on ice before addition or refrigerate prior to use.*

*Optional: Incubate crude lysate for 5 minutes on ice*

16 mL

24 mL

Proceed with step 8 of the high copy plasmid purification protocol (section 7.1) if not significantly more than the recommended lysis buffer volumes were used.

Otherwise it might be advantageous to centrifuge the precipitate first in order to avoid clogging of the NucleoBond® Xtra Column Filters.

## 7.3 Concentration of NucleoBond® Xtra eluates with NucleoBond® Finalizers

*Note:* Use of the **NucleoBond® Finalizers** is only recommended for vector sizes smaller than 50 kbp.

Midi – NucleoBond®  
Finalizer

Maxi – NucleoBond®  
Finalizer Large

### 1 Precipitation

*Note:* Check DNA concentration photometrically before precipitation. This helps to choose the best buffer volume in step 5 and allows calculation of the recovery after concentration.

Add **0.7 volumes** of **room-temperature isopropanol** (not supplied with the kit). Vortex well and let the mixture sit for **2 minutes**.

(E.g., for 5 mL NucleoBond® Xtra Midi eluate add **3.5 mL** isopropanol, for 15 mL NucleoBond® Xtra Maxi eluate add **10.5 mL** isopropanol)

**3.5 mL for  
5 mL eluate**

**10.5 mL for  
15 mL eluate**

### 2 Loading

Remove the plunger from a **30 mL Syringe** and attach a NucleoBond® Finalizer to the outlet. Add the precipitation mixture into the syringe, insert the plunger, hold the syringe in a vertical position, and press the mixture **slowly** through the NucleoBond® Finalizer (the mixture should pass the NucleoBond® Finalizer drop by drop). Discard the flow-through.

### 3 Washing

Remove the NucleoBond® Finalizer from the syringe, pull out the plunger and reattach the NucleoBond® Finalizer to the syringe outlet.

Add **70 % ethanol** (not supplied with the kit) into the syringe, insert the plunger, hold the syringe in a vertical position, and press the ethanol **slowly** through the NucleoBond® Finalizer. Discard the flow-through.

**2 mL**

**4 mL**

### 4 Drying

Remove the NucleoBond® Finalizer from the syringe, pull out the plunger and reattach the NucleoBond® Finalizer. Press air through the NucleoBond® Finalizer as strongly as possible while **touching a tissue** with the tip of the NucleoBond® Finalizer to soak up ethanol.

Repeat this step at least as often as indicated below until **no more ethanol** leaks from the NucleoBond® Finalizer.

*Note:* A new dry syringe can be used to speed up the procedure (not provided).

**≥ 6 times until dry**

**≥ 6 times until dry**

Midi – NucleoBond®  
FinalizerMaxi – NucleoBond®  
Finalizer Large

*Optional: You can incubate the NucleoBond® Finalizer for 10 minutes at 80 °C to minimize ethanol carry-over. However, the final recovery may be reduced by over-drying the DNA.*

---

## 5 Elution (Buffer TRIS)

Remove the NucleoBond® Finalizer from the syringe, pull out the plunger of a **1 mL Syringe** and attach the NucleoBond® Finalizer to the syringe outlet.

*Note: Refer to section 4.13, Table 4 (Midi) or Table 5 (Maxi) to choose the appropriate volume of elution buffer.*

Pipette an appropriate volume of **Redissolving Buffer TRIS** (5 mM Tris/HCl, pH 8.5) or TE buffer into the syringe (see section 4.13). Do not use pure water unless pH is definitely higher than 7.0. Place the **NucleoBond® Finalizer** outlet in a vertical position over a fresh collection tube (not provided) and **elute plasmid DNA very slowly** drop by drop by inserting the plunger.

200 – 800 µL

400 – 1000 µL

Remove the NucleoBond® Finalizer from the syringe, pull out the plunger and reattach the NucleoBond® Finalizer to the syringe outlet.

**Transfer the first eluate back into the syringe and elute into the same collection tube a second time.**

**Load first eluate completely****Load first eluate completely**

For very large expected yields (> 400 µg NucleoBond® Xtra Midi; > 1000 µg NucleoBond® Xtra Maxi) recovery can be increased by a third round of elution.

Remove the NucleoBond® Finalizer from the syringe, pull out the plunger to aspirate air, reattach the NucleoBond® Finalizer and **press the air out again to force out as much eluate as possible.**

Determine plasmid yield by UV spectroscopy and confirm plasmid integrity by agarose gel electrophoresis (see section 4.14).

---

## 8 Appendix

### 8.1 Troubleshooting

If you experience problems with reduced yield or purity, it is recommended to check which purification step of the procedure is causing the problem.

**First**, the bacterial culture has to be checked for sufficient growth ( $OD_{600}$ ) in the presence of an appropriate selective antibiotic (Table 1, section 4.13). **Second**, aliquots of the cleared lysate, the flow-through, the combined washing steps (Buffer EQU and Buffer WASH), and the eluate should be kept for further analysis by agarose gel electrophoresis.

Refer to Table 6 to choose a fraction volume yielding approximately 5 µg of plasmid DNA assuming 250 µg and 1000 µg were loaded onto the **NucleoBond® Xtra Midi** and **Maxi Column**, respectively. Precipitate the nucleic acids by adding 0.7 volumes of isopropanol, centrifuge the sample, wash the pellet using 70 % ethanol, centrifuge again, remove supernatant, air dry for 10 minutes, dissolve the DNA in 100 µL TE buffer, pH 8.0, and run 20 µL on a 1 % agarose gel.

**Table 6: NucleoBond® Xtra eluate volumes required for an analytical check**

| Sample | Purification step                              | Volume required [µL] |      |
|--------|--|----------------------|------|
|        |  | Midi                 | Maxi |
| I      | Cleared lysate of protocol step 8              | 500                  | 200  |
| II     | Column flow-through after protocol step 8      | 500                  | 200  |
| III    | Wash flow-through after protocol step 9 and 11 | 250                  | 200  |
| IV     | Eluate after protocol step 12                  | 100                  | 100  |


The exemplary gel picture (Figure 6) will help you to address the specific questions outlined in the following section more quickly and efficiently.

It shows for example the dominant plasmid bands which should only be present in the eluate and in the lysate before loading to proof plasmid production in your cell culture (lane 1). Plasmid DNA found in the wash fractions, however, narrows down the problem to wrong or bad wash

buffers (e. g., wrong pH, buffer components precipitated, evaporation of liquid due to wrong storage).

RNA might be visible as a broad band at the bottom of the gel for the lysate and the lysate flow-through samples (lanes 1 and 2). It might also occur in the wash fraction but must be absent in the eluate.

Genomic DNA should not be visible at all but would show up in the gel slot or right below indicating for example too harsh lysis conditions.

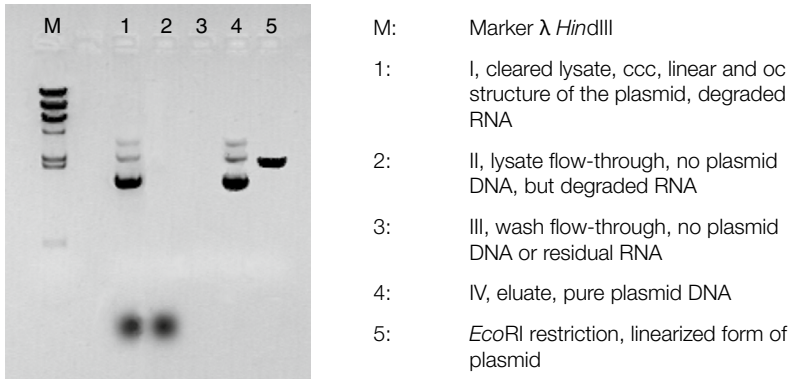

**Figure 6 Exemplary analytical check of NucleoBond® Xtra Midi purification samples**

Plasmid: pUC18, bacterial strain: *E. coli* DH5 $\alpha$ ®. 20  $\mu$ L of each precipitated sample has been analyzed on a 1 % agarose gel. Equal amounts of plasmid DNA before (lane 1) and after (lane 4) purification using NucleoBond® Xtra Midi are shown with a recovery of > 90 %.

| Problem | Possible cause and suggestions |
|---------|--------------------------------|
|---------|--------------------------------|

*Plasmid did not propagate*

- Check plasmid content in the cleared lysate (see Figure 6). Use colonies from fresh plates for inoculation and add fresh selective antibiotic to plates and media.
- Estimate plasmid content prior to large purifications by a quick NucleoSpin® Plasmid or NucleoSpin® Plasmid EasyPure preparation.

*Alkaline lysis was inefficient*

- Too much cell mass was used. Refer to section 4.5 4.8 regarding recommended culture volumes and lysis buffer volumes. Check plasmid content in the cleared lysate (see Figure 6).
- Check Buffer LYS for SDS precipitation before use, especially after storage below 20 °C. If necessary incubate the bottle for several minutes at 30–40 °C and mix well until SDS is redissolved.

*SDS- or other precipitates are present in the sample*

- Load the crude lysate onto the NucleoBond® Xtra Column Filter inserted in the NucleoBond® Xtra Column. This ensures complete removal of SDS precipitates. Incubation of cleared lysates for longer periods of time might lead to formation of new precipitate. If precipitate is visible, it is recommended to filter and centrifuge the lysate again directly before loading it onto the NucleoBond® Xtra Column.

No or low  
plasmid DNA  
yield

*Sample/lysate is too viscous*

- Too much cell mass was used. Refer to section 4.5 4.8 regarding recommended culture volumes and lysis buffer volumes.
- Make sure to mix well after neutralization to completely precipitate SDS and chromosomal DNA. Otherwise, filtration efficiency and flow rate go down and SDS prevents DNA from binding to the column.

*pH or salt concentrations of buffers are too high*

- Check plasmid content in the wash fractions (see Figure 6). Keep all buffers tightly closed. Check and adjust pH of Buffer EQU (pH 6.5), WASH (pH 7.0), and ELU (pH 9.0) with HCl or NaOH if necessary.

| Problem  | Possible cause and suggestions   |  |
|--|--|--|
| NucleoBond®<br>Xtra Column<br>Filter clogs<br>during filtra-tion | <p data-bbox="300 209 568 231"><i>Culture volumes are too large</i></p> <ul data-bbox="300 252 978 300" style="list-style-type: none"> <li>• Refer to section 4.5 4.8 regarding recommended culture volumes and larger lysis buffer volumes.</li> </ul> <p data-bbox="300 320 736 343"><i>Precipitate was not resuspended before loading</i></p> <ul data-bbox="300 363 863 386" style="list-style-type: none"> <li>• Invert crude lysate at least 3 times directly before loading.</li> </ul> <p data-bbox="300 406 564 429"><i>Incomplete precipitation step</i></p> <ul data-bbox="300 450 941 488" style="list-style-type: none"> <li>• Make sure to mix well after neutralization to completely precipitate SDS and chromosomal DNA.</li> </ul> |  |
|  | NucleoBond®<br>Xtra Column is<br>blocked or very<br>slow   | <p data-bbox="300 512 499 534"><i>Sample is too viscous</i></p> <ul data-bbox="300 555 958 770" style="list-style-type: none"> <li>• Do NOT attempt to purify lysate prepared from a culture volume larger than recommended for any given column size with standard lysis buffer volumes. Incomplete lysis not only blocks the column but can also significantly reduce yields. Refer to section 4.5 and 4.6 for recommended culture volumes and section 4.8 for larger culture volumes and adjusted lysis buffer volumes.</li> <li>• Make sure to mix well after neutralization to completely precipitate SDS and chromosomal DNA.</li> </ul> |
|  |  | <p data-bbox="300 791 614 813"><i>Lysate was not cleared completely</i></p> <ul data-bbox="300 834 969 943" style="list-style-type: none"> <li>• Use NucleoBond® Xtra Column Filter or centrifuge at higher speed or for a longer period of time.</li> <li>• Precipitates occur during storage. Clear lysate again before loading the column.</li> </ul>   |
| Genomic DNA<br>contamination<br>of plasmid DNA                   | <p data-bbox="300 967 575 989"><i>Lysis treatment was too harsh</i></p> <ul data-bbox="300 1010 848 1031" style="list-style-type: none"> <li>• Make sure not to lyse in Buffer LYS for more than 5 min.</li> </ul>   |  |
|  | <p data-bbox="300 1051 796 1074"><i>Lysate was mixed too vigorously or vortexed after lysis</i></p> <ul data-bbox="300 1094 975 1153" style="list-style-type: none"> <li>• Invert tube for only 5 times. Do not vortex after addition of Buffer LYS.</li> <li>• Use larger tubes or reduce culture volumes for easier mixing.</li> </ul>   |  |

| Problem   | Possible cause and suggestions   |
|---|--|
| RNA contamination of plasmid DNA                  | <p><i>RNase digestion was inefficient</i></p> <ul style="list-style-type: none"> <li>• RNase was not added to Buffer RES or stored improperly. Add new RNase to Buffer RES. See section 8.2 for ordering information.</li> </ul> <p><i>pH or salt concentration of wash buffer is too low</i></p> <ul style="list-style-type: none"> <li>• Check RNA content in the wash fractions (see Figure 6). Keep all buffers tightly closed. Check pH of Buffer EQU (pH 6.5) and WASH (pH 7.0) and adjust with HCl or NaOH if necessary.</li> <li>• Increase wash buffer stringency by adjusting pH of Buffer WASH to 7.5.</li> </ul> |
|   | <p><i>Wash step with Buffer WASH was not sufficient</i></p> <ul style="list-style-type: none"> <li>• Double or triple washing step with Buffer WASH. Additional Buffer WASH can be ordered separately (see ordering information).</li> </ul>   |
| Low purity ( $A_{260}/A_{280} < 1.8$ )            | <p><i>NucleoBond® Xtra Column Filter was not removed before second washing step</i></p> <ul style="list-style-type: none"> <li>• Protein content too high due to inefficient washing. Remove the NucleoBond® Xtra Column Filter <b>before</b> performing the second washing step with Buffer WASH.</li> </ul>  |
|   | <p><i>Buffer WASH was used instead of Buffer EQU for the first wash</i></p> <ul style="list-style-type: none"> <li>• Buffer EQU has to be used to wash out the NucleoBond® Xtra Column Filter to avoid SDS carry-over.</li> </ul> <p><i>Only minimal amounts of DNA were loaded onto the column</i></p> <ul style="list-style-type: none"> <li>• Excess free binding capacity requires more extensive washing – double washing step with Buffer WASH.</li> <li>• Reduce lysis time &lt; 5 min.</li> </ul>  |
| No nucleic acid pellet formed after precipitation | <p><i>Pellet was lost</i></p> <ul style="list-style-type: none"> <li>• Handle the precipitate with care. Decant solutions carefully. Determine DNA yield in Buffer ELU in order to calculate the amount of plasmid DNA that should be recovered after precipitation.</li> </ul>  |
|   | <p><i>Plasmid DNA might be smeared over the wall of the tube</i></p> <ul style="list-style-type: none"> <li>• Dissolve DNA with an appropriate volume of reconstitution buffer by rolling the tube for at least 30 min.</li> </ul> <p><i>Nucleic acid did not precipitate</i></p> <ul style="list-style-type: none"> <li>• Check type and volumes of precipitating solvent. Make sure to use at least 0.7 volumes of isopropanol and mix thoroughly.</li> <li>• Centrifuge for longer periods of time at high speed.</li> </ul>  |

| Problem   | Possible cause and suggestions   |
|---|--|
| <p>Nucleic acid pellet is opaque or white instead of clear and glassy</p> | <p><i>Co-precipitation of salt</i></p>   |
|   | <ul style="list-style-type: none"> <li>• Check isopropanol purity, and perform precipitation at room temperature but centrifuge at 4 °C. Do not let the eluate drip from the column into isopropanol but add isopropanol to the final eluate and mix immediately.</li> <li>• Try resuspending the pellet in Buffer WASH, and reload onto the same NucleoBond® Xtra Column. Wash the column several times with Buffer WASH before loading.</li> </ul> |
| <p>Nucleic acid pellet does not resuspend in buffer</p>                   | <p><i>Pellet was over-dried</i></p>  |
|   | <ul style="list-style-type: none"> <li>• Try to dissolve at higher temperatures for a longer period of time (e. g., 2 h at 37 °C or overnight at RT), preferably under constant spinning (3D-shaker).</li> </ul>   |
|   | <p><i>Co-precipitation of salt or residual alcohol</i></p>   |
| <p>Nucleic acid pellet does not resuspend in buffer</p>                   | <ul style="list-style-type: none"> <li>• Wash the pellet again with 70 % ethanol, or increase the reconstitution buffer volume.</li> </ul>   |
|   | <p><i>Insoluble particles in redissolved DNA</i></p>   |
| <p>Nucleic acid pellet does not resuspend in buffer</p>                   | <ul style="list-style-type: none"> <li>• Centrifuge the redissolved DNA to pellet the insoluble particles and transfer supernatant to a new tube. Insoluble particles do not affect DNA quality. As an alternative insoluble particles can easily be removed by using the NucleoBond® Finalizer (NucleoBond® Xtra Midi) or NucleoBond® Finalizer Large (NucleoBond® Xtra Maxi).</li> </ul>   |

---

**Problem**      **Possible cause and suggestions**

---

*Already no or low plasmid DNA after elution from the NucleoBond® Xtra Column*

- Refer to detailed troubleshooting “No or low plasmid DNA yield”.

*Dead volume too high*

- If high concentration of plasmid DNA is the main priority, elution should be performed in small volumes. Naturally a portion of the eluate will be lost in the syringe and on the NucleoBond® Finalizer. To minimize these losses in the second elution step, try to transfer even the last droplet from the syringe to the NucleoBond® Finalizer, for example by tapping the NucleoBond® Finalizer and syringe onto the bench top. Then fill the syringe with air and press forcefully the last droplets out of the NucleoBond® Finalizer. Repeat this step several times. You might have to practice this procedure several times to achieve optimal results. An acceptable dead volume is smaller than 30 µL with NucleoBond® Finalizer and 60 µL with NucleoBond® Finalizer Large.

*Elution volume too small*

No or low plasmid DNA yield after NucleoBond® Finalizer precipitation

- Since there are dead volumes of about 30 µL (NucleoBond® Finalizer) and 60 µL (NucleoBond® Finalizer Large), reasonable elution volumes start with 200 µL (NucleoBond® Finalizer) and 400 µL (NucleoBond® Finalizer Large) respectively. Further-more, smaller volumes are insufficient to wet the entire membrane and will drastically decrease your yield. Refer to section 4.13, Table 4 and Table 5 to estimate the recovery that can be expected depending on elution buffer volume.

*Elution too fast*

- Plasmid DNA needs time to dissolve. Elute really very slowly, drop by drop. Repeat the elution procedure using the first eluate.

*Forgot to elute a second time*

- Repeating the elution procedure with the first eluate is crucial for optimal yields. However, eluting a third time shows no further improvement.

*Plasmid size*

- Precipitation efficiency is almost independent of plasmid size, but elution from the NucleoBond® Finalizers becomes more and more difficult with increasing size of the construct. If you face low yields with large cosmids you may try heating the NucleoBond® Finalizer, the syringes, and elution buffer to 70 °C.
-

---

**Problem**                      **Possible cause and suggestions**

---

|   |   |
|---|---|
| Low DNA concentration after NucleoBond® Finalizer precipitation | <p data-bbox="291 201 448 231"><i>Low overall yield</i></p> <ul data-bbox="291 239 978 327" style="list-style-type: none"><li data-bbox="291 239 978 327">• Refer to detailed troubleshooting “No or low plasmid DNA yield” and lower your elution buffer volume. Refer to section 4.13, Table 4 and Table 5 to estimate the DNA concentrations that can be expected.</li></ul> <p data-bbox="291 335 784 367"><i>Fresh elution buffer was used for second elution step</i></p> <ul data-bbox="291 375 978 462" style="list-style-type: none"><li data-bbox="291 375 978 462">• The second elution step is crucial for optimal yield but to achieve a high DNA concentration the eluate of the first elution step has to be used for the second elution.</li></ul> <p data-bbox="291 470 526 502"><i>Not enough DNA loaded</i></p> <ul data-bbox="291 510 978 702" style="list-style-type: none"><li data-bbox="291 510 978 702">• Since there is a technical limitation to at least 200 µL (NucleoBond® Finalizer) and 400 µL (NucleoBond® Finalizer Large) of elution buffer due to membrane wetting and dead volume, a minimal amount of DNA has to be loaded to achieve a desired concentration. If possible try to pool several DNA precipitation batches since percentage of recovery and concentration significantly increase with higher amounts of loaded DNA.</li></ul> |
| Low recovery when using the Finalizer                           | <p data-bbox="291 710 649 742"><i>Resuspension time might be too short</i></p> <ul data-bbox="291 750 978 1192" style="list-style-type: none"><li data-bbox="291 750 978 1192">• Depending on the total amount of the precipitated plasmid it will need some time to redissolve completely. Resuspension time might be too short for a complete recovery, if the redissolving buffer is passed by the precipitated plasmid on the Finalizer membrane too quickly. If a high recovery is mandatory it is recommended to incubate the precipitated plasmid in the redissolving buffer during the elution step. Therefore, do not press the elution buffer through the Finalizer in one rush, but rather stop pressing the buffer through as soon as the first drops have passed the outlet. Let the redissolving buffer sit on the membrane in the Finalizer for 5 minutes at room temperature before completing the elution step. Reload the eluate onto the Finalizer and repeat the procedure at least once. General recommendations are also valid here: push the redissolving buffer through the membrane slowly, increase the elution volume to gain a higher recovery and blow out the dead volume completely by pushing air through the Finalizer.</li></ul>  |

---

| <b>Problem</b>   | <b>Possible cause and suggestions</b>  |
|--|--|
| Purified plasmid does not perform well in subsequent reactions | <i>Plasmid DNA is contaminated with chromosomal DNA or RNA</i>   |
|  | <ul style="list-style-type: none"> <li>Refer to the detailed troubleshooting above.</li> </ul>   |
|  | <i>Plasmid DNA is contaminated with residual alcohol</i>   |
|  | <ul style="list-style-type: none"> <li>Plasmid DNA was not dried completely before redissolving. Precipitate DNA again by adding 1/10 volume of 3 M NaAc pH 5.0 and 0.7 volumes of isopropanol. Proceed with the precipitation protocol in this manual and dry DNA pellet completely.</li> </ul> |
|  | <i>DNA is degraded</i>   |
|  | <ul style="list-style-type: none"> <li>Make sure that your entire equipment (pipettes, centrifuge tubes, etc.) is clean and nuclease-free.</li> <li>Do not lyse the sample with Buffer LYS for more than 5 min.</li> </ul>   |
|  | <i>DNA is irreversibly denatured</i>   |
|  | <ul style="list-style-type: none"> <li>A denatured plasmid band runs faster on the gel than the supercoiled conformation. Do not lyse the sample after addition of Buffer LYS for more than 5 minutes.</li> </ul>  |

## 8.2 Ordering information

| <b>Product</b>   | <b>REF</b>         | <b>Pack of</b>  |
|--|--------------------|-----------------|
| NucleoBond® Xtra Midi  | 740410.10/.50/.100 | 10/50/100 preps |
| NucleoBond® Xtra Midi Plus (incl. NucleoBond® Finalizers)  | 740412.10/.50      | 10/50 preps     |
| NucleoBond® Xtra Maxi  | 740414.10/.50/.100 | 10/50/100 preps |
| NucleoBond® Xtra Maxi Plus (incl. NucleoBond® Finalizers Large)  | 740416.10/.50      | 10/50 preps     |
| NucleoBond® Xtra Combi Rack  | 740415             | 1               |
| NucleoBond® Xtra Buffer Set I (Buffer RES, LYS (with LyseControl), NEU, RNase A; only applicable with NucleoBond® Xtra kits; sufficient for 12 Xtra Maxi and 18 Xtra Midi preps) | 740417             | 1               |
| Buffer RES   | 740363.1000        | 1000 mL         |
| Buffer EQU   | 740317.1000        | 1000 mL         |
| Buffer WASH  | 740375.1000        | 1000 mL         |

| Product  | REF                 | Pack of                             |
|--|---------------------|-------------------------------------|
| Buffer ELU   | 740316.600          | 600 mL                              |
| NucleoBond® Finalizer<br>(for use with NucleoBond® Xtra Midi, Midi EF, NucleoBond® PC 100, PC 500, PC 500 EF)      | 740519.20           | 20 filters<br>2 syringe sets        |
| NucleoBond® Finalizer Plus<br>(for use with NucleoBond® Xtra Midi, Midi EF, NucleoBond® PC 100, PC 500, PC 500 EF) | 740520.20           | 20 filters<br>20 syringe sets       |
| NucleoBond® Finalizer Large<br>(for use with NucleoBond® Xtra Maxi, Maxi EF, NucleoBond® PC 2000, PC 2000 EF)      | 740418.20           | 20 large filters<br>2 syringe sets  |
| NucleoBond® Finalizer Large Plus<br>(for use with NucleoBond® Xtra Maxi, Maxi EF, NucleoBond® PC 2000, PC 2000 EF) | 740419.20           | 20 large filters<br>20 syringe sets |
| RNase A (lyophilized)  | 740505.50<br>740505 | 50 mg<br>100 mg                     |
| NucleoMag® Desalting Beads<br>(for desalting of NucleoBond® eluates)   | 744410.50           | 4 x 1.5 mL and Buffer TRIS (60 mL)  |

Visit [www.mn-net.com](http://www.mn-net.com) for more detailed product information.

### 8.3 Product use restriction / warranty

All MACHEREY-NAGEL products are designed for their intended use only. They are not intended to be used for any other purpose. The description of the intended use of the products can be found in the original MACHEREY-NAGEL product leaflets. Before using our products, please observe the instructions for use and the safety instructions from the respective Material Safety Data Sheet of the product.

This MACHEREY-NAGEL product is carrying documentation stating specifications and other technical information. MACHEREY-NAGEL warrants to meet the stated specifications. The provided warranty is limited to the data specifications and descriptions as given in the original MACHEREY-NAGEL literature. No other statements or representations, written or oral, by MACHEREY-NAGEL's employees, agents or representatives, except written statements signed by a duly authorized officer of MACHEREY-NAGEL are authorized. They should not be relied upon by the customer and are not a part of a contract of sale or of this warranty.

Liability for all possible damages that occur in any connection with our products is limited to the utmost minimum as stated in the general business terms and conditions of MACHEREY-NAGEL in their latest edition which can be taken from the company's website. MACHEREY-NAGEL does not assume any further warranty.

Products and their application are subject to change. Therefore, please contact our Technical Service Team for the latest information on MACHEREY-NAGEL products. You may also contact your local distributor for general scientific information. Descriptions in MACHEREY-NAGEL literature are provided for informational purposes only.

Last updated: 08/2022, Rev. 04

Please contact:  
MACHEREY-NAGEL GmbH & Co. KG  
Tel.: +49 24 21 969-333  
support@mn-net.com


---

**Trademarks:**

DH5 $\alpha$ <sup>®</sup> is a trademark of Life Technologies, Inc.

NucleoSpin<sup>®</sup> is a trademark of MACHEREY-NAGEL GmbH & Co. KG

NucleoBond<sup>®</sup> is a trademark of MACHEREY-NAGEL GmbH & Co. KG.

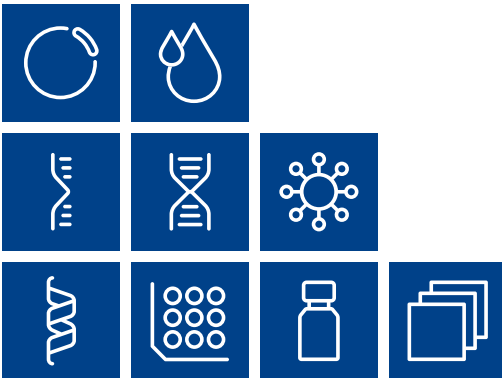

Plasmid DNA

Clean up

RNA

DNA


Viral RNA and DNA

Protein

High throughput

Accessories

Auxiliary tools

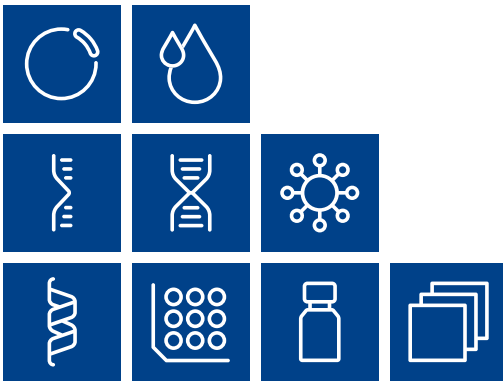

# MACHEREY-NAGEL

[www.mn-net.com](http://www.mn-net.com)

MACHEREY-NAGEL GmbH & Co. KG · Valencienner Str. 11 · 52355 Düren · Germany

DE +49 24 21 969-0 [info@mn-net.com](mailto:info@mn-net.com)

CH +41 62 388 55 00 [sales-ch@mn-net.com](mailto:sales-ch@mn-net.com)

FR +33 388 68 22 68 [sales-fr@mn-net.com](mailto:sales-fr@mn-net.com)

US +1 888 321 62 24 [sales-us@mn-net.com](mailto:sales-us@mn-net.com)

